



OWNER'S MANUAL

4040-650/4070-650
POWER EXAM TABLE



SERIAL NUMBER

DATE OF MANUFACTURE

MAXIMUM PATIENT WEIGHT 650 LBS / 295 KG

IMPORTANT INFORMATION

Safety First: This equipment must be operated and maintained with the safety of the patient and doctor in mind.

- 1 Read this manual before operating your new UMF Medical equipment.
- 2 This product is intended to be used for positioning of patients during medical examinations conducted by qualified medical personnel.
- 3 This manual should remain permanently affixed or near the equipment for convenient reference.
- 4 UMF Medical reserves the right to make changes to the design of products at any time and without notice.

CLASSIFICATIONS

Equipment Class – Class I

Protection against electric shock: Type B applied parts

Protection against harmful ingress of water: Ordinary Equipment is not suitable for use in the presence of a flammable anesthetic mixture with air or with oxygen or with nitrous oxide .

Mode of Operation: Continuous operation with intermittent loading 1 minute on 9 minutes off or 2 minutes on, 18 minutes off.

This product has been evaluated with respect to electrical shock, fire, & mechanical hazards only, in accordance with UL60601-1 and CAN/CSA-22.2 No. 601.1



* Label found on back of table

SAFETY SYMBOLS

WARNING: The warning symbol identifies special instructions or procedures, which if not correctly followed could result in personal injury.

CAUTION: The caution symbol identifies special instructions or procedures, which if not properly followed could result in danger or damage to equipment.



UL CLASSIFICATION MARK WITH RESPECT TO ELECTRIC SHOCK, FIRE AND MECHANICAL HAZARDS ONLY IN ACCORDANCE WITH UL60601-1.



ATTENTION, CONSULT ACCOMPANYING DOCUMENTS



TYPE B APPLIED PART

ENVIRONMENTAL CONDITIONS





TRANSPORT/STORAGE TEMPERATURE: -20°C to 40°C

TRANSPORT/STORAGE/OPERATING HUMIDITY: 95% maximum

OPERATING TEMPERATURE: 0°C to 40°C





SPECIFICATIONS (4040-650)

Maximum Patient Weight	650 lbs (295 kg)
Electrical Supply(Standard)	120V 60HZ 9AMP
Electrical Supply(Optional)	220V 60HZ 5AMP
Power Cord Length	10 FT (3.0m)
Table Weight	400 lbs (181kg)
Paper Roll (Maximum size)	21.0" Long x 3.5" Diameter (53.3 cm x 8.9 cm)
Storage Drawer (Front)	19.0" W x 12.0" D x 3.5" H (48 cm x 30 cm x 9 cm)
Storage Drawer (Side)	24.5" W x 12.5" D x 3.5" H (62 cm x 32 cm x 9 cm)

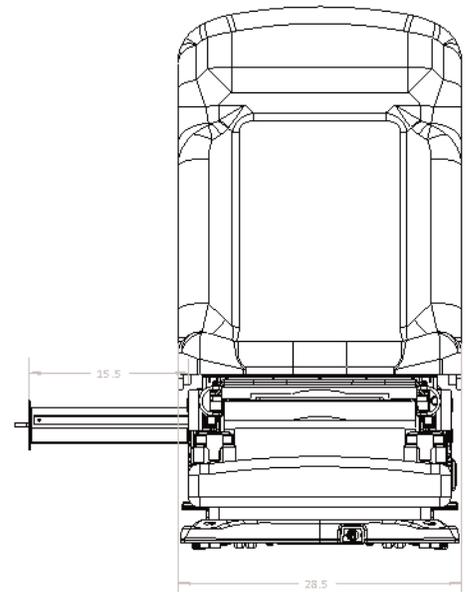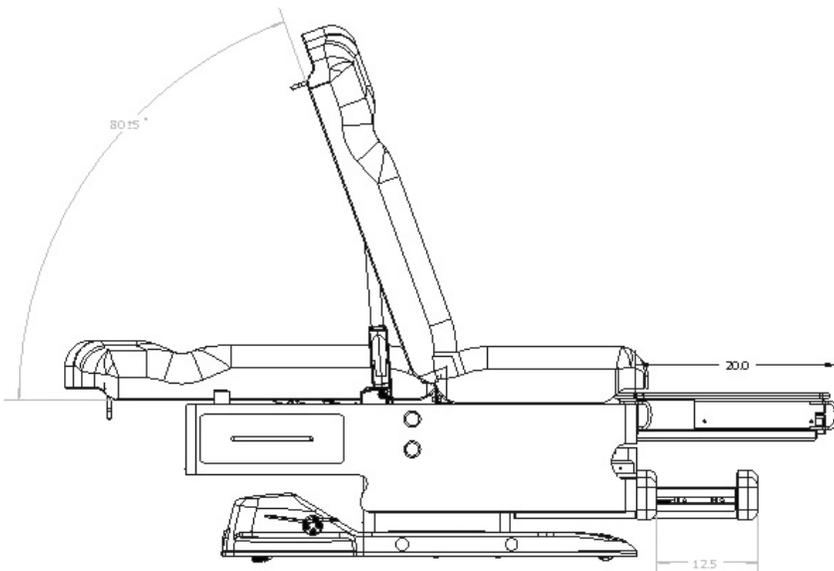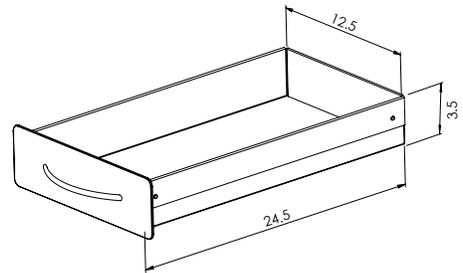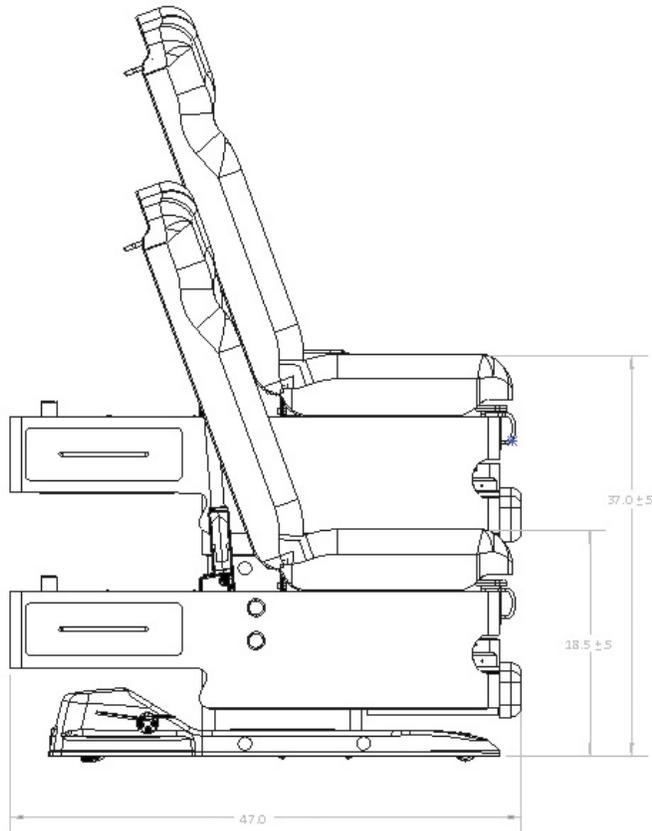

SPECIFICATIONS (4070-650)

Maximum Patient Weight	650 lbs (295 kg)
Electrical Supply(Standard)	120V 60HZ 9AMP
Electrical Supply(Optional)	220V 60HZ 5AMP
Power Cord Length	10 FT (3.0m)
Table Weight	400 lbs (181kg)
Paper Roll (Maximum size)	21.0" Long x 3.5" Diameter (53.3 cm x 8.9 cm)
Storage Drawer (Front)	19.0" W x 12.0" D x 3.5" H (48 cm x 30 cm x 9 cm)
Storage Drawer (Side)	24.5" W x 12.5" D x 3.5" H (62 cm x 32 cm x 9 cm)

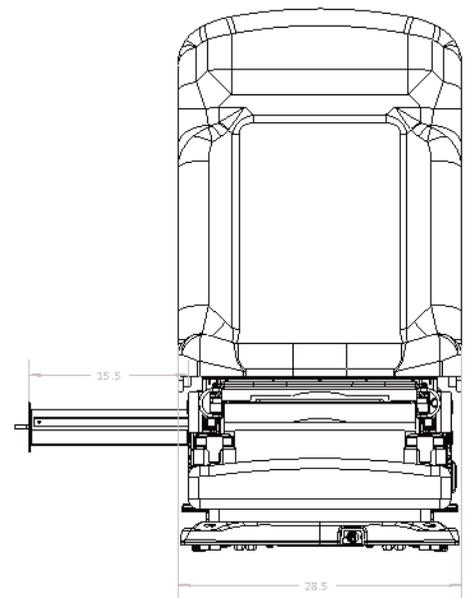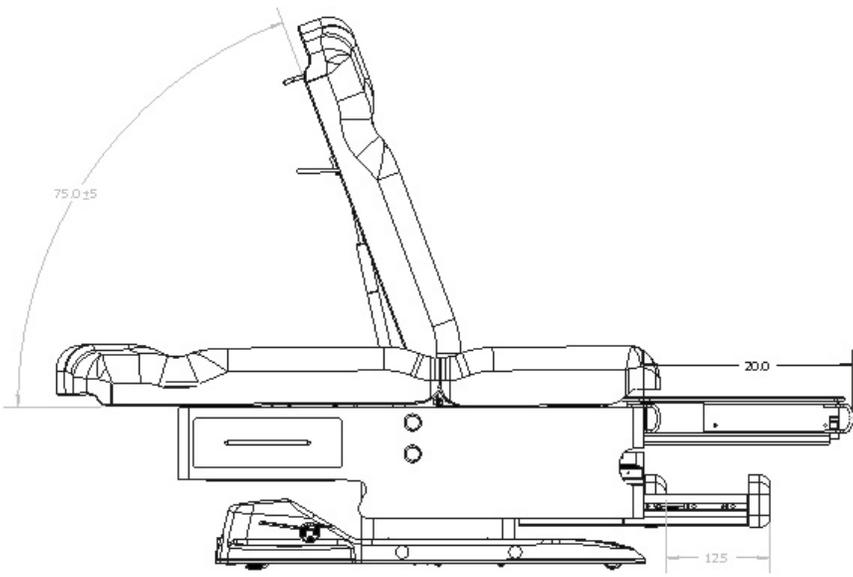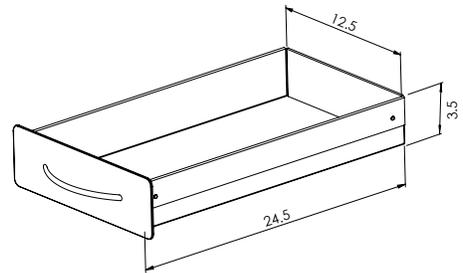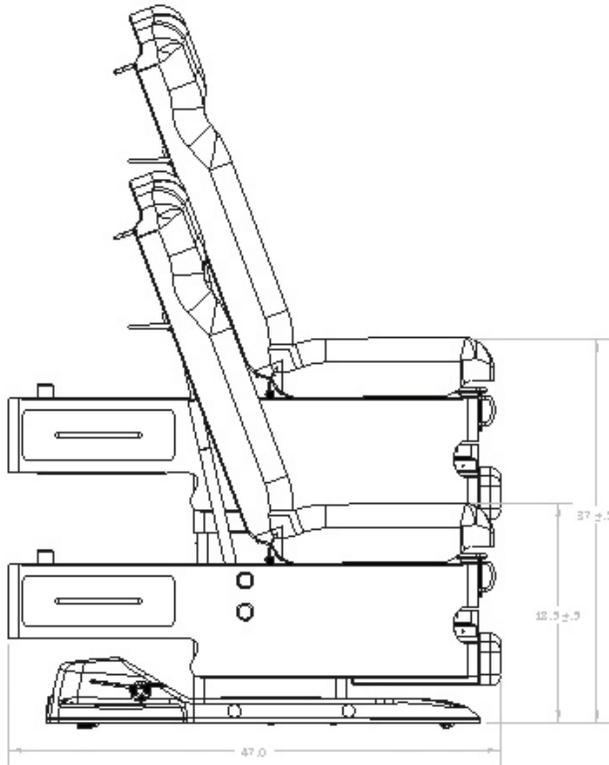

SAFETY FEATURES

Patient Safety Table Lockout



This table is equipped with a safety feature that allows the practitioner to deactivate all table functions in order to prevent misuse when staff is not present.

To lock and unlock:	Press & hold STOP button for 2 seconds.	1 beep indicates locked 2 beeps indicates unlocked
---------------------	-----------------------------------------	-------------------------------------------------------


WARNING: FOR MAXIMUM PATIENT SAFETY, LOCK TABLE IMMEDIATELY AFTER EACH USE

FEATURES AND OPERATION

Hand & Foot Control – Table Operation (4040-650)



Hand Control

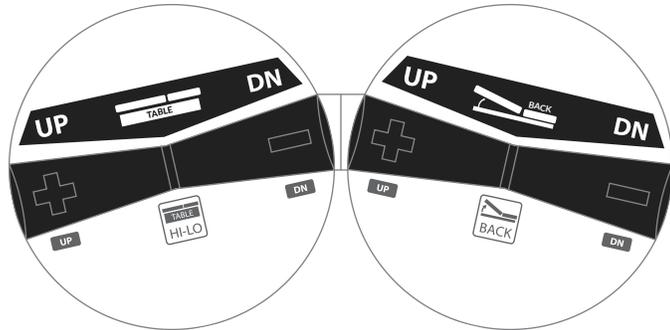

Foot Control



Height Adjustment



Home



Backrest Adjustment


WARNING: DO NOT USE BACKREST AS A SEAT

FEATURES AND OPERATION

Hand & Foot Control – Table Operation (4070-650)



Hand Control

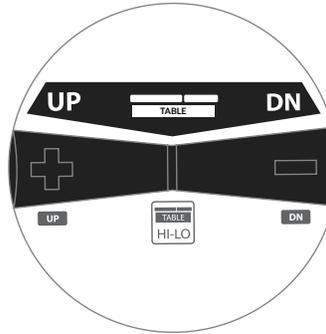


Foot Control



Height Adjustment



Home

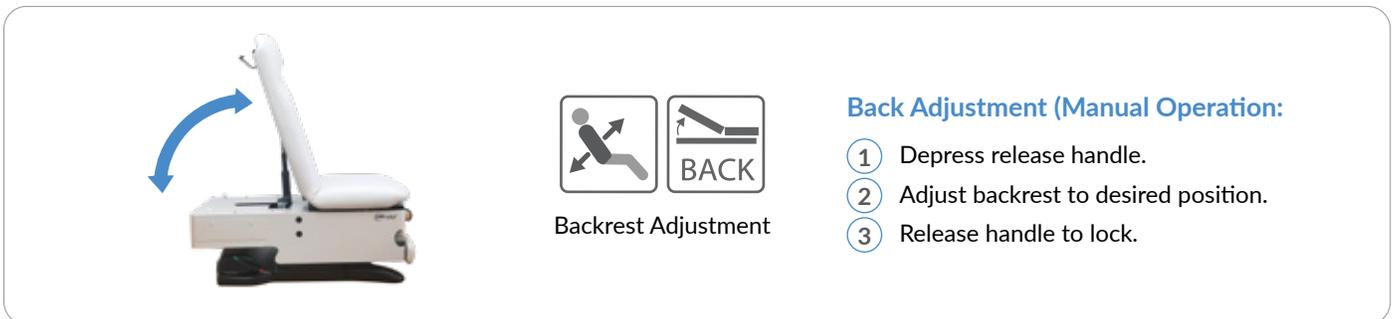

Backrest Adjustment


Back Adjustment (Manual Operation:

- 1 Depress release handle.
- 2 Adjust backrest to desired position.
- 3 Release handle to lock.

WARNING: DO NOT USE BACKREST AS A SEAT

FEATURES AND OPERATION

Hand Control – Memory Programming & Special Functions

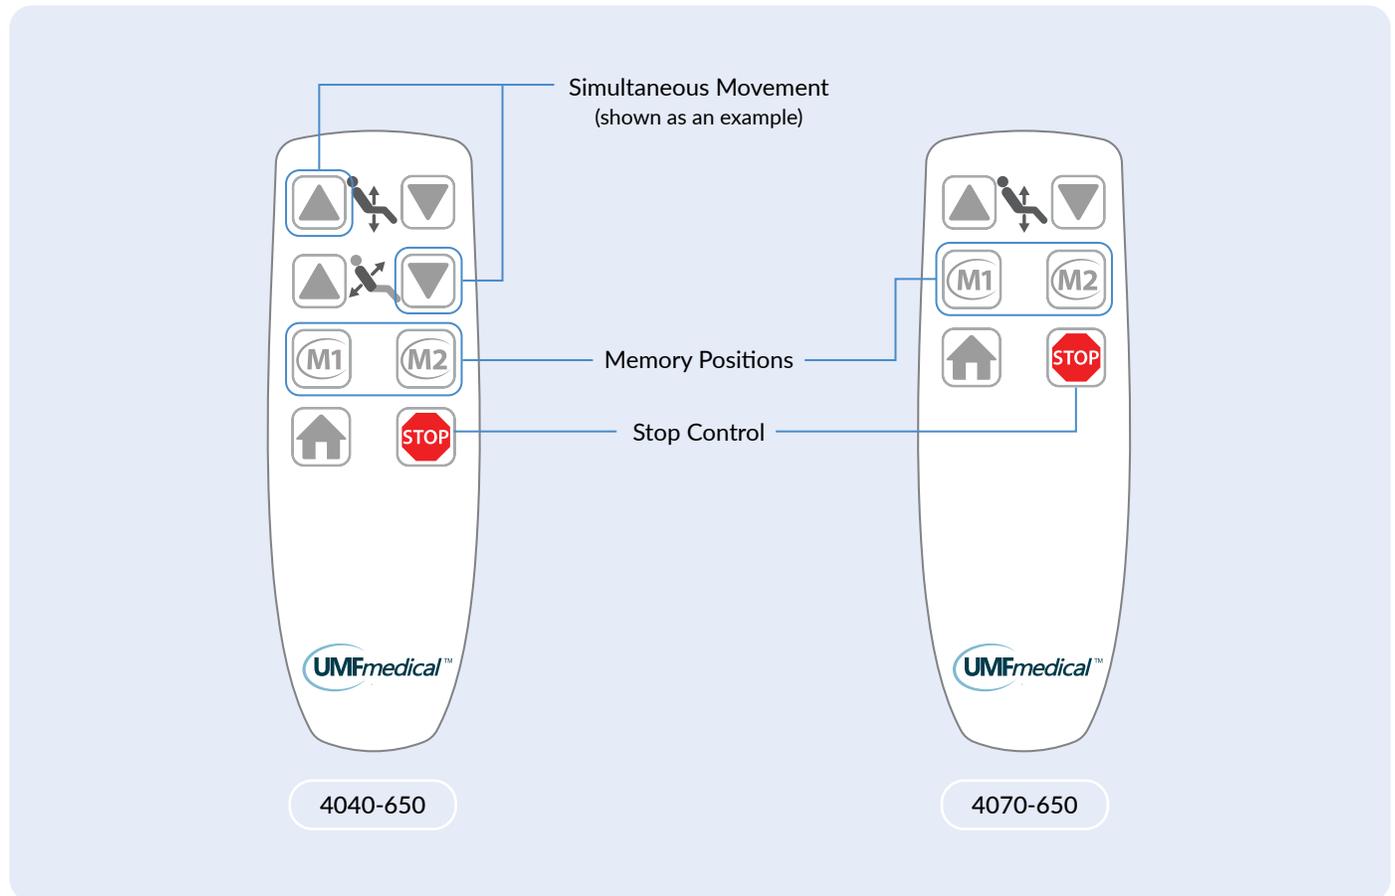

  – Two programmable positions for storing commonly use table positions.

To Program:

- 1 Move table to desired position for memory storage.
- 2 Press and hold (approximately 3 seconds) desired memory position button (M1 or M2) in which table position is to be stored. An audible double beep should be heard indicating table position has been programmed.
- 3 To use memory function, press and hold the memory button (M1 or M2) for 1 second. Table will return to programmed position.

Holding the memory button (M1 or M2) for 3 seconds when performing step 3 will cause the memory button to re-program to the current position of the table.

 – Stops table movement when any impulse movements (HOME, Memory Function M1 or M2) are being used. Pressing any button on the hand or foot control will cancel table movement.

Simultaneous movement

- › Press any combination of buttons for simultaneous movement of multiple functions

FEATURES AND OPERATION

Removable Upholstered Top (Installation)



Step 1:

Carefully lay upholstered top on table, aligning black slide latches on underside of upholstery with cutouts in support pan.



Step 2:

Slide latches may not be perfectly aligned when upholstery is resting on the support pan. Proceed to next step.



Step 3:

If latches are not properly aligned, slightly raise foot section and maneuver upholstery slightly until all latches align properly.



Step 4:

Raise the back section of the upholstery and support pan (4070-650:) by squeezing the manual release lever and gently lifting upward. (4040-650:) by using hand or foot control.



Step 5:

Using your index finger, slide all four black slide latches toward the center of the support pan until fully engaged. Lower the back section.



Step 6:

Raise the foot section of the upholstery and support pan, and repeat the step five for the remaining four black slide latches. Lower the foot section.

Removable Upholstered Top (Removal)




Step 1:

Grasp slide latch with thumb and forefinger.



Step 2:

Pull the slide latch toward you (away from the metal pan).

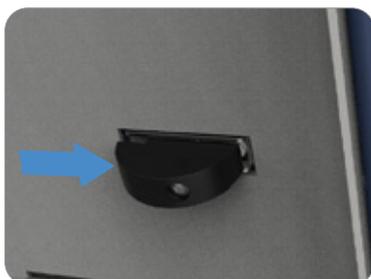

Step 3:

While pulling toward you (away from the pan), slide the latch to the unlocked position.



Step 4:

Allow the latch to return to its normal position. Repeat for all latches.

FEATURES AND OPERATION

Storage Drawers



Side Drawer
24.5" x 12.5" x 3.5"
(62cm x 32cm x 9cm)



Front Drawer
19.0" x 12.0" x 3.5"
(48cm x 30cm x 9cm)

Leg Extension & Drip Pan



- 1 Slide the leg section out.
- 2 Lift front of the leg pad to disengage from locked position.
- 3 Slide leg pad toward rear of table.

WARNING: DO NOT USE THE LEG REST TO SUPPORT PATIENT'S ENTIRE WEIGHT.

Leg Rest Pad



- 1 Slide pad forward until it makes contact with the two pins toward the front of the leg section
- 2 Lift the front of the leg pad until it clears the two pins and pull the leg pad forward.
- 3 Lower the front of the leg pad. The two pins will enter slots located on the bottom of the leg pad, preventing movement.

CAUTION: WITH LEG REST PAD IN TILTED POSITION, THE FRONT SLIDE PINS ON PAD MUST SEAT AGAINST BUMPER STOPS IN THE LEG SECTION. THE TILT SUPPORTS MUST BE FULLY EXTENDED FROM UNDERNEATH PAD.

FEATURES AND OPERATION

Paper Roll Replacement



Max Roll Size
21" x 3.5" (53cm x 9cm)

Slide rod out of brackets, install new roll, and reinstall into brackets

Stirrup Positioning & Adjustment



- 1 Pull the stirrups out and unfold.
- 2 Lift slightly and move left or right to position.
- 3 Release stirrup to lock into position.

WARNING: DO NOT SUPPORT THE PATIENT'S ENTIRE WEIGHT WITH THE STIRRUPS.

Pelvic Tilt



- 1 Lift up seat section and flip the pelvic support arm.
- 2 Place seat section down to secure the mechanism.

FEATURES AND OPERATION

Reversing Side Drawers



Step 1:
Remove side panels.



Step 2:
Remove drawer

- › Extend drawer
- › Press tabs on both sides
- › Remove drawer



Step 3:
Slide cages to opposite side of table.



Step 4:
Align slides and install drawer on opposite side.
* Slide in until an audible "click!" is heard.



Step 5:
Install side panel on opposite side.

COMMON OPTIONS AND ACCESSORIES

Mobile Caster Base (142)

Concealed retractable casters can be installed on base to allow for easy table movement for cleaning.



Table in
LOCKED position



Table in UNLOCKED in
cleaning position

WARNING: TABLE IS NOT TO BE USED FOR PATIENT TRANSPORT. ENSURE WHEELS ARE IN 'PATIENT READY' POSITION PRIOR TO A PATIENT ACCESSING TABLE.

WARNING: TABLE IS NOT TO BE USED FOR PATIENT TRANSPORT. CASTERS ARE TO BE USED SOLELY WHEN MOVING TABLE WITHIN THE EXAMINATION ROOM TO FACILITATE CLEANING UNDERNEATH THE TABLE. CASTERS ARE NOT TO BE USED DURING INSTALLATION OR FOR TRANSPORT INSIDE OR OUTSIDE OF FACILITY.

CAUTION: LOW GROUND CLEARANCE WHEN TABLE IS ENGAGED IN CLEANING POSITION. AVOID ROLLING TABLE OVER OBJECTS GREATER THAN .25" HIGH OR DAMAGE MAY OCCUR.

Drawer Warmer (850)



① Press switch to power on and off.

COMMON OPTIONS AND ACCESSORIES

Hospital Grade Receptacle with Child Safe Cover (852)



- 1 To access receptacles, insert a screwdriver, key, or other tool into slot on receptacle cover to remove child-proof cover.
- 2 Replace child-proof cover following use.

Option available on the 200 series and standard on the 300 series.

WARNING: OUTLET IS FOR MEDICAL EQUIPMENT ONLY.
CAUTION: CHECK GROUND CONTINUITY PERIODICALLY.
120V MAXIMUM OUTPUT - 5.0A, 120V
220V MAXIMUM OUTPUT - 2.5A, 220V

WARNING: DO NOT DISCARD COVER. COVER IS TO BE REAPPLIED AFTER REMOVAL OF EQUIPMENT FROM MULTIPLE SOCKET OUTLET.

WARNING: MULTIPLE SOCKET OUTLET IS TO BE USED FOR MEDICAL EQUIPMENT ONLY (WHERE SAFETY CERTIFICATION HAS BEEN PERFORMED IN ACCORDANCE TO IEC 60601-1 AND/OR IEC 60601-1-1). USE OF EQUIPMENT NOT COMPLYING WITH THE EQUIVALENT SAFETY REQUIREMENT OF THIS EQUIPMENT MAY LEAD TO A REDUCED LEVEL OF SAFETY OF THE RESULTING SYSTEM.

WARNING: GROUND RELIABILITY CAN ONLY BE ACHIEVED WHEN POWER SUPPLY IS CONNECTED TO AN EQUIVALENT RECEPTACLE MARKED "HOSPITAL ONLY" OR "HOSPITAL GRADE".

Service Note: If the maximum load of the receptacle is exceeded, two circuit breakers will interrupt power. To reset, toggle the far two circuit breakers located behind the receptacle outlet box in the back of the drawer panel.

COMMON OPTIONS AND ACCESSORIES

Bierhoff Knee Crutch (251-Pair)



- 1 Extend stirrups to full-extended position with heel stirrup in retracted position.
- 2 Insert knurled end of knee crutch rod into hole on end of stirrup.
- 3 Adjust to position and tighten with slide lock.

Stainless Steel Irrigation Pan with Spout (822)



The stainless steel drain pan is offered without a spout (standard) or with spout (optional - shown left) for the procedure that you need.

CABLE CONNECTION



ATTENTION:
If hand control will be primary control used, UMF Medical recommends the hand control to be plugged into the front of the table.

Front
① Optional port for foot or hand control.

Back (Left to Right)
① Port for foot control.
② Port for hand control.
③ LED
④ Port for power cord

Cable Locking Feature



- ① Plug into the hand control port.
- ② Turn the union nut clockwise until fully threaded.



- ① Plug into the hand control port.
- ② Turn the union nut clockwise until fully threaded.

* Union nut has a slit in it to allow for easy threading.

Upholstery with PreFixx® Protective Finish

Helping to enhance infection prevention initiatives

In laboratory testing, upholstery protected with PreFixx® finish was treated with the following disinfectants with little to no discoloration or damage to the upholstery. This testing may not reflect actual results in the field.*

Recommended Disinfectants**

- › Ecolab Quaternary Disinfectant Wipes
- › Agar™ Powerquat
- › Asepticare™
- › Asepticare™ TB-II
- › AVISTAT-D™ Ready To Use Spray Disinfectant Cleaner
- › Biotrol BirexSE®
- › Bleach 1:5 (20% bleach)
- › Bleach 1:9 (10% bleach)
- › Bleach-Rite® Disinfecting Spray
- › CaviCide™
- › CaviCide1™
- › CaviCide™ AF
- › Clorox® Broad Spectrum Quaternary Disinfectant Cleaner
- › Clorox® Healthcare Bleach Germicidal Cleaner
- › Clorox® Healthcare Bleach Germicidal Wipes
- › Clorox® Healthcare EZ-KILL® Wipes
- › Clorox® Healthcare VersaSure® Cleaner Disinfection Wipes
- › Clorox® Hydrogen Peroxide Cleaner Disinfectant Spray
- › Clorox® Hydrogen Peroxide Cleaner Disinfectant Wipes
- › Diversey™ Accel® INTERvention® Wipes
- › Diversey™ Avert® Sporicidal Disinfectant Cleaner
- › ERC Performance Wipes
- › McKesson Disposable Germicidal Surface Wipes
- › McKesson Pro-Tech RTU Disinfectant Cleaner
- › OPTIM® 1 Wipes
- › OPTIM® 33TB
- › Oxivir® 1 RTU
- › Oxivir® Five 16
- › Oxivir® TB
- › OxyCide™ Daily Disinfectant Cleaner
- › PDI Sani-Cloth® AF3 Germicidal Disposable Wipes
- › PDI Sani-Cloth® HB
- › PDI Sani-Cloth® Plus
- › PDI Sani-Cloth® Prime Germicidal Disposable Wipe
- › PDI Super Sani-Cloth®
- › PDI Super Sani-Cloth® Bleach Germicidal Disposable Wipes
- › Precise QTB Spray
- › PROCHEM® Oxy Plus
- › Purell® Healthcare Surface Disinfectant
- › Purell® Multi-Surface Disinfectant
- › Sani Professional® Cleaning + Degreasing Multi-Surface Wipes
- › Sani Professional® Multi-Surface Cleaning Wipes
- › Sani Professional® No-Rinse Sanitizing Multi-Surface Wipes
- › SaniZide® Plus
- › STERI-7 XTRA CONCENTRATE (recommended dilution ratio 1:10)
- › STERI-7 XTRA WIPES
- › Vert-2-Go ED
- › Virox AHP 5
- › Virox PREempt™ RTU
- › Virex® II 256
- › Virex® Plus One-Step Disinfectant Cleaner & Deodorant
- › Wayne® Concept 256N
- › Wex-Cide 128

**All disinfectants and cleaning agents contain chemicals that degrade coated fabric upholstery to some extent. To promote a long product life, it is recommended that the PreFixx cleaning and maintenance protocol be employed regularly.*

***Recommended disinfectants are only recommended when following the disinfectant manufacturer's instructions for application, and inclusion in this document does not imply "fit for use." Customers should first determine if products are appropriate for use on their surfaces.*



Care & Cleaning

Use one of the following cleaners with a soft cloth or damp sponge. Rinse area with fresh water then dry with a clean, lint-free cloth.

Primary Recommended Cleaner

- › Formula 409 All-Purpose spray cleaner

Secondary Recommended Cleaners

- › Lysol Clean and Fresh Multi-Surface Cleaner (Reckitt Benckiser)
- › Lestoil Heavy Duty Cleaner (Clorox)
- › Mr. Clean / Flash Clean and Shine (Procter and Gamble)
- › Eco Touch All Purpose Premium Care
- › Mr. Clean Magic Eraser Original

For more difficult stains, contact UMF Medical Customer Service.

EQUIPMENT CARE

Care of upholstery

The upholstery material used on the top, leg rest, and headrest is resistant to most medical stains.

For light cleaning:

- 1 A solution of 10% liquid soap and clean water applied with a soft damp cloth will remove disinfection cleaner build-up.
- 2 If necessary, a solution of liquid cleanser and water can be applied with a soft bristle brush. Wipe away residue with a water-dampened cloth.

For disinfection:

- 1 Dampen a soft white cloth with a solution of standard bleach (sodium hypochlorite) or other chlorine-based cleaner*** and water; 10% bleach, 90% water.
- 2 Rub gently.
- 3 If necessary, allow the 1:10 diluted bleach (sodium hypochlorite) solution to puddle on the affected area or apply with a clean, soaked cloth for approximately 30 minutes. Rinse with a water-dampened cloth to remove any remaining bleach concentration.
- 4 Rinse with a water-dampened cloth to remove cleaner solution and allow thorough drying of material.

***See current CDC Guideline for Disinfection & Sterilization in Healthcare Facilities for bleach alternative cleaners.

Note: Immediately remove any fluid spilled on upholstery surface.

Antimicrobial: UMF Medical Upholstery provides outstanding protection in difficult medical and healthcare environments and contains an agent effective against bacterial and fungal microorganisms.

Care of painted surfaces

A chemical acid-resistant paint is used, but extreme care must be taken not to use ammonia-based cleaners or discoloration of paint may occur. A damp cloth or mild liquid soap solution should be sufficient.

Care of bright metal surfaces

All non-painted surfaces, chrome plated, or stainless steel should be wiped weekly with a clean damp cloth then buffed to a lustrous shine with a soft dry cloth.

Care of base

The protective base is easily washable with mild liquid soap and water. A soft bristle brush may be used on scuffed or stained areas.

CAUTION: WHEN THE USE OF STRONG CLEANING SOLUTIONS IS NECESSARY, TEST AN INCONSPICUOUS AREA TO ASSURE THAT DAMAGE TO UPHOLSTERY OR PAINTED SURFACES WILL NOT OCCUR.

QUESTIONS, COMMENTS OR SERVICE REQUESTS

Contact:

UMF Medical Customer Service
1316 Eisenhower Blvd
Johnstown, PA 15904

Toll Free: 1(800) 638-5322
Email: customerservice@umfmedical.com
Fax: 1(814) 266-1870

* For service requests, please have model % serial number available.

WARRANTY INFORMATION

UMF Medical warrants to the original purchaser a warranty for products to be free from functional defects in material and workmanship under normal interior use and service. UMF Medical's obligation under this warranty is limited to the repair or replacement, at UMF Medical's option, of the parts or the products the defects of which are reported to UMF Medical within the applicable warranty period and which upon examination by UMF Medical prove to be defective. Warranty subject to the terms and conditions listed below.

Length of warranty, measured by Purchase Date (Invoice Date), for all warranted products and components:

- Five years:* Signature Series Examination Tables (52xx model numbers and Treatment and Orthopedic Tables (55xx model numbers). Ultra-Comfort adjustable backrest cylinder not included.
- Three years:* Power Exam and Procedure Tables and all other UMF Medical products excluding the products listed in Five Year and One Year categories of this document.
- One year:* Waste Receptacles, Bassinet Baskets, Bassinet Mattresses and ultra-comfort adjustable backrest cylinder.

Obtaining Warranty Service

Warranty service must be obtained by contacting either the Authorized Distributor through whom the product was purchased or UMF Medical Customer Service Department via phone at 814-266-8726, or via email at customerservice@umfmedical.com.

This warranty covers the cost associated with the repair parts only and does not cover any other charges, including but not limited to service calls, labor, transportation, shipping, etc. It is the retail customer's obligation to arrange delivery of a product to UMF Medical or one of its authorized distributors for warranty service, which delivery shall be at the retail purchaser's expense. It is also the retail purchaser's obligation to comply with the warranty service instruction provided by UMF Medical or its authorized distributor. The retail purchaser must provide UMF Medical with completed warranty registration information within thirty days after purchase in order to obtain the benefits of this warranty.

Limited warranty general exceptions and exclusions

This warranty does not cover and UMF Medical shall not be liable for the following:

- › Parts and products of a consumable nature;
- › Defects, damage or other conditions caused, in whole or in part, by mishandling, misuse, abuse, negligence, alteration,

accident, freight damage, tampering or failure to seek and obtain repair or replacement in a timely manner;

- › Products which are not installed, used, and properly cleaned and maintained as required in the UMF Medical installation and/or Owner's Manual for the applicable product;
- › Replacement parts, alterations or installation of any accessories or parts not manufactured or recommended by UMF Medical;
- › Cosmetic and non-functional defects not noted at time of delivery.
- › Charges for repairs, replacement parts, adjustments, installation or other work performed upon or in connection with products which are not expressly authorized in writing in advance by UMF Medical.
- › Damages resulting from inadequate power supply (including incorrect voltage, voltage spikes or other irregularities) or use or storage in corrosive atmospheres.

To the extent any or all of the following exclusions or provisions of this warranty are prohibited by any federal, state, or municipal law which cannot be preempted, those exclusions or provisions shall not be applicable.

Exclusive Remedy: Consequential Damages Disclaimer

UMF Medical's only obligation under this warranty is the repair or replacement of defective parts. UMF Medical shall not be liable for and hereby disclaims any direct, special, indirect, incidental, exemplary or consequential damages or delays, including but not limited to, damages for loss of profits or income, loss of use, downtime, employee or independent contractor wages, payments and benefits, commercial loss or other incidental charges.

No Authorization

No person or firm is authorized to create or approve for UMF Medical any other obligation or liability in connection with the products.

Warranty Disclaimer

THIS WARRANTY IS UMF MEDICAL'S ONLY WARRANTY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED. UMF MEDICAL MAKES NO IMPLIED WARRANTIES OF ANY KIND INCLUDING ANY IMPLIED WARRANTIES OR MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. THIS WARRANTY IS LIMITED TO THE REPAIR OR REPLACEMENT OF DEFECTIVE PARTS.

No action may be brought against UMF Medical for breach of this limited warranty, an implied warranty, if any, or for any other claim arising out of or relating to the products following expiration of the limited warranty period.

UMF Medical reserves the right to make changes in the design or material of its products without incurring any obligation to incorporate such changes in any product previously manufactured.

SETUP INSTRUCTIONS

Models 4040/4070-650-100 (Power100+, Power 100)

To set up your New Power Table:

PLEASE FOLLOW THESE STEPS COMPLETELY to ensure that your table functions properly PLEASE DO NOT PLUG TABLE IN UNTIL PRECEDING STEPS ARE COMPLETED.

1. The table has one (1) port for the foot control in the front of the table base.
2. Locate the plug port in the front of the table base.
3. Locate green dot on the left side of the port.
4. Locate green dot on the plug end of the foot control.
5. Align green dot on plug with green dot on port.
6. Plug in foot control completely, ensuring that yellow 'O' ring is completely inserted into the port until the yellow color completely disappears.
NOTE: IF YELLOW O-RING IS NOT COMPLETELY INSERTED INTO THE PORT, THE TABLE WILL NOT FUNCTION. THE TABLE WILL BEEP AND REQUIRE A CONTROL BOX RESET. THIS IS A SAFETY FEATURE.
7. Slide the round crew lock forward over the port plug and turn clockwise to tighten. Ensure completely tight.
8. Plug power cord into the port in the exam table.

Models 4040/4070-650-200 & 300 (Power200+, Power 200, ProGlide300+, ProGlide300)

To set up your New Power Table:

PLEASE FOLLOW THESE STEPS COMPLETELY to ensure that your table functions properly PLEASE DO NOT PLUG TABLE IN UNTIL PRECEDING STEPS ARE COMPLETED.

1. The table has three (3) ports for the hand and foot control in the table base: two (2) located at the rear and one (1) located at the front.
2. Locate the ports and choose which ports you prefer to place hand and foot controls.
3. Start with installing the hand control.
4. Locate the green dot on the port on the table base.
5. Locate green dot on the plug end of the hand control.
6. Align green dot on plug with green dot on port.
7. Plug in hand control completely, ensuring that yellow 'O' ring is completely inserted into the port until the yellow color completely disappears.
NOTE: IF YELLOW O-RING IS NOT COMPLETELY INSERTED INTO THE PORT, THE TABLE WILL NOT FUNCTION. THE TABLE WILL BEEP AND REQUIRE A CONTROL BOX RESET. THIS IS A SAFETY FEATURE.
8. Slide the round crew lock forward over the port plug and turn clockwise to tighten. Ensure completely tight.
9. Choose the port in the front or rear of the table for your foot control.
10. Locate green dot on the port.
11. Locate green dot on the plug end of the foot control.
12. Align green dot on plug with green dot on port.
13. Plug in foot control completely, ensuring that yellow 'O' ring is completely inserted into the port until the yellow color completely disappears.